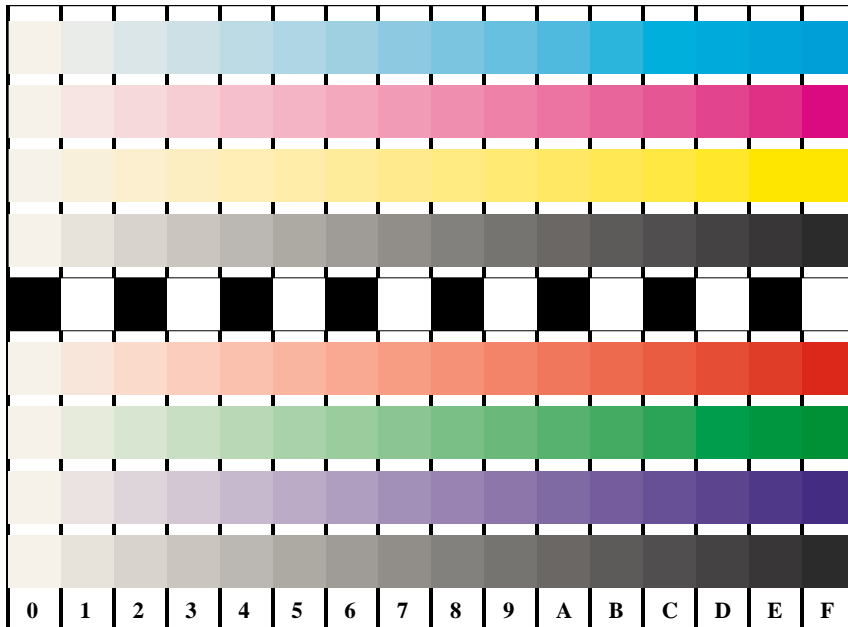


C
 LAB^* M
 LAB^* Y
 LAB^* N
 LAB^* O
 LAB^* L
 LAB^* V
 LAB^* N
 LAB^* Figure B4 and D4 of the ISO/IEC-test charts no. 2 and 4; 16 visual equidistant steps of colour series; Use of the PS operator LAB^* setcolorFig. B4 of ISO/IEC-test chart 2 and
Fig. D4 of ISO/IEC-test chart no. 4;ISO/IEC 15775 and
TR ISO/IEC 24705;input: LAB^* setcolor
output: no change compared to input