


http://130.149.60.45/~farbmetrik/LE80/LE80L0N1.TXT /PS; start output
N: No Output Linearization (OL) data in File (F), Startup (S) or Device (D)

See original or copy: http://web.me.com/Klaus_richter/LE80/LE80L0N1.TXT /PS
Technical information: <http://www.ps.bam.de> or <http://130.149.60.45/~farbmetrik>

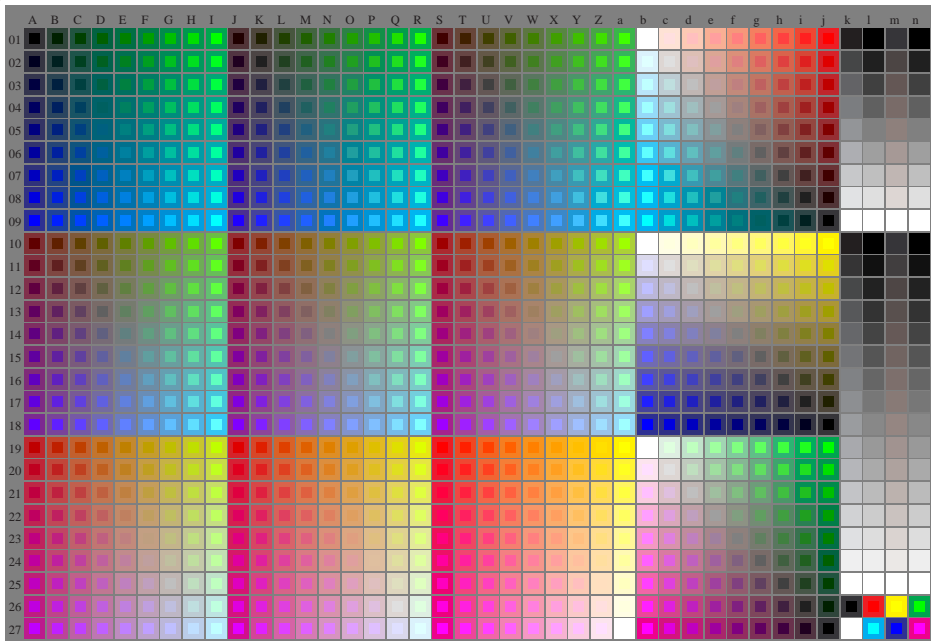

TUB registration: 20110301-LE80/LE80L0N1.TXT /PS
application for measurement of printer or monitor systems

TUB material: code=rhata

LE800-7N, 1/3, Test chart G with 40x27=1080 colours; digital equidistant 9 or 16 step colour scales; Colour data in column (A-n): $cm\dot{y}0 + rgb(A_j + k26_n27), 000n(k), w(l), nnn0(m), www(n), colorm = 0, separation = A$

TUB-test chart LE80; Colorimetric system G, Page 1/1
40x27=1080 colours for Measurement: $cm\dot{y}0/000n/w/nnn0/www$ input: $cm\dot{y}0/000n/w/nnn0/www$ output: no change compared to input