



















TUB registration: 20241001-heb6/heb6On1.txt /ps application for evaluation and measurement of dispersion

TUB material: code=rha4ta

<http://farbe.li.tu-berlin.de/heb6/heb6l0n1.txt> /ps; only vector graphic VG; start output
see separate images of this page: <http://farbe.li.tu-berlin.de/heb6/heb6.htm>

see separate images of this page: <http://farbe.li.tu-berlin.de/heb6/heb6.htm>

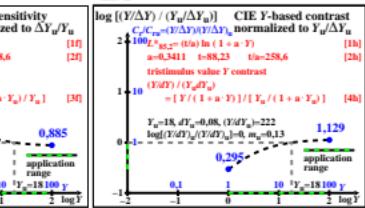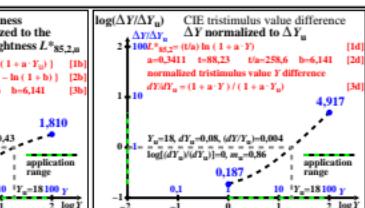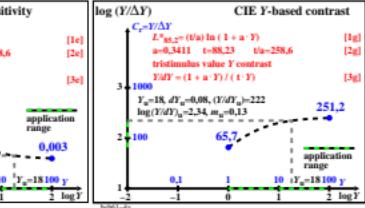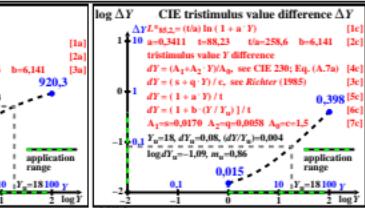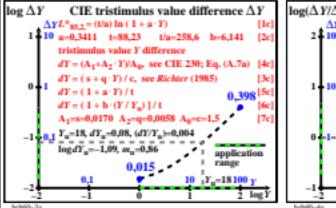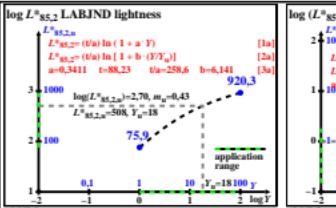

TUB-test chart heb6; Calculated for the CIELAB colour-difference formula, see ISO/CIE 11664-4
 log[lightness L^* , threshold ΔY , sensitivity $\Delta Y/Y$, contrast $Y/\Delta Y$, unnormalized and normalized]