
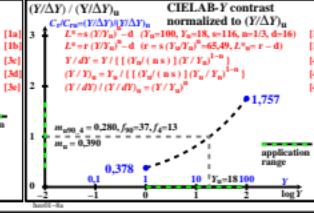
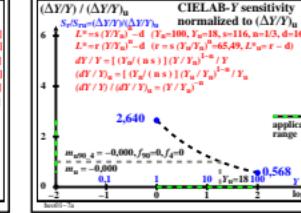
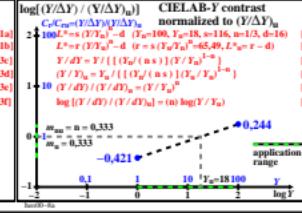

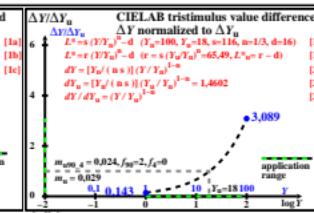
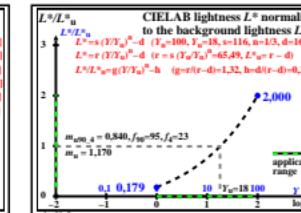
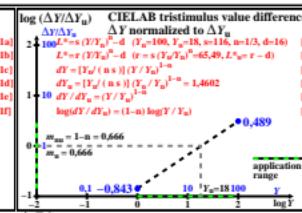

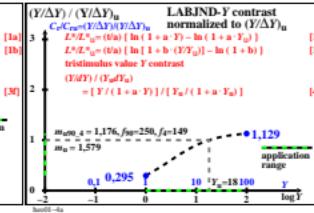
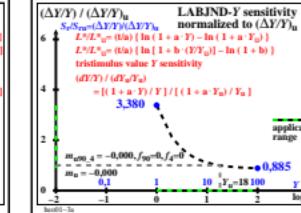
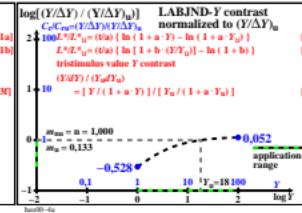

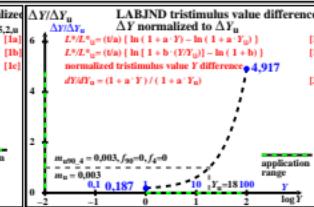
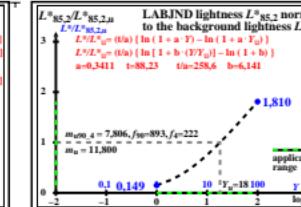
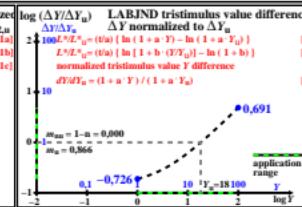


application for evaluation and measurement of display or print output

<http://farbe.li.tu-berlin.de/heo0/heo0ln1.txt/.ps>; only vector graphic VG; start output  
see separate images of this page: <http://farbe.li.tu-berlin.de/heo0/heo0.htm>

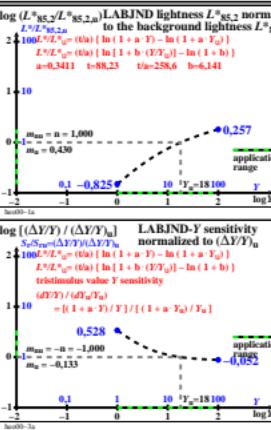

TUB-test chart heo0; LABJND & CIELAB colour-difference, CIE 230 & ISO/CIE 11664-4  
log & lin[lightness  $L^*$ , threshold  $\Delta Y$ , sensitivity  $\Delta Y/Y$ , contrast  $Y/Y$ , normalized for grey U]